

SEMINARIO TALLER PARA DETERMINAR VIDA UTIL

09-Vida-Util.xls
ASPIRADOR QUIRURGICO

	VIDA UTIL SIN MANTENIMIENTO			VIDA UTIL CON MANTENIMIENTO		
	1a. Ronda	2a. Ronda	3a. Ronda	1a. Ronda	2a. Ronda	3a. Ronda
1	1	-	-	15	5	-
2	1	-	-	14	5	-
3	1	-	-	10	5	-
4	1	-	-	10	5	-
5	1	-	-	10	5	-
6	1	-	-	4	5	-
7	1	-	-	3	5	-
8	1	-	-	3	10	-
9	1	-	-	5	10	-
10	1	-	-	5	10	-
11	1	-	-	5	10	-
12	1	-	-	5	10	-
13	1	-	-	5	10	-
14	1	-	-	5	10	-
15	1	-	-	5	10	-
16	1	-	-	5	10	-
17	1	-	-	5	10	-
18	1	-	-	-	15	-
19	3	-	-	-	-	-
20	-	-	-	-	-	-
21	-	-	-	-	-	-
22	-	-	-	-	-	-
23	-	-	-	-	-	-
24	-	-	-	-	-	-
25	-	-	-	-	-	-
26	-	-	-	-	-	-
27	-	-	-	-	-	-
28	-	-	-	-	-	-
29	-	-	-	-	-	-

SEMINARIO TALLER PARA DETERMINAR VIDA UTIL


09-Vida-Util.xls
ASPIRADOR QUIRURGICO

ASPIRADOR QUIRURGICO


	VIDA UTIL SIN MANTENIMIENTO			VIDA UTIL CON MANTENIMIENTO		
	1a. Ronda	2a. Ronda	3a. Ronda	1a. Ronda	2a. Ronda	3a. Ronda
MEDIA	1.105263158			6.70588235	8.33333333	
DESVIACION	0.458831468			3.67023	2.97044263	
MODA	1			5	10	
MEDIANA	1			5	10	

1	18	1	0	1	0	
2	0	2	0	2	0	
3	1	3	0	3	0	
4	0	4	0	4	0	
5	0	5	0	5	7	
6	0	6	0	6	0	
7	0	7	0	7	0	
8	0	8	0	8	0	
9	0	9	0	9	0	
10	0	10	0	10	10	
11	0	11	0	11	0	
12	0	12	0	12	0	
13	0	13	0	13	0	
14	0	14	0	14	0	
15	0	15	0	15	1	
16	0	16	0	16	0	
17	0	17	0	17	0	
18	0	18	0	18	0	
19	0	19	0	19	0	
20 O MAS	0	20 O MAS	0	20 O MAS	0	
	1	0	1	0	1	0
	2	0	2	0	2	0
	3	0	3	2	3	0
	4	0	4	1	4	0
	5	0	5	9	5	0
	6	0	6	0	6	0
	7	0	7	0	7	0
	8	0	8	0	8	0
	9	0	9	0	9	0
	10	0	10	3	10	0
	11	0	11	0	11	0
	12	0	12	0	12	0
	13	0	13	0	13	0
	14	0	14	1	14	0
	15	0	15	1	15	0
	16	0	16	0	16	0
	17	0	17	0	17	0
	18	0	18	0	18	0
	19	0	19	0	19	0
20 O MAS		0	20 O MAS		0	20 O MAS


ASPIRADOR SIN MANTENIMIENTO RONDA-1

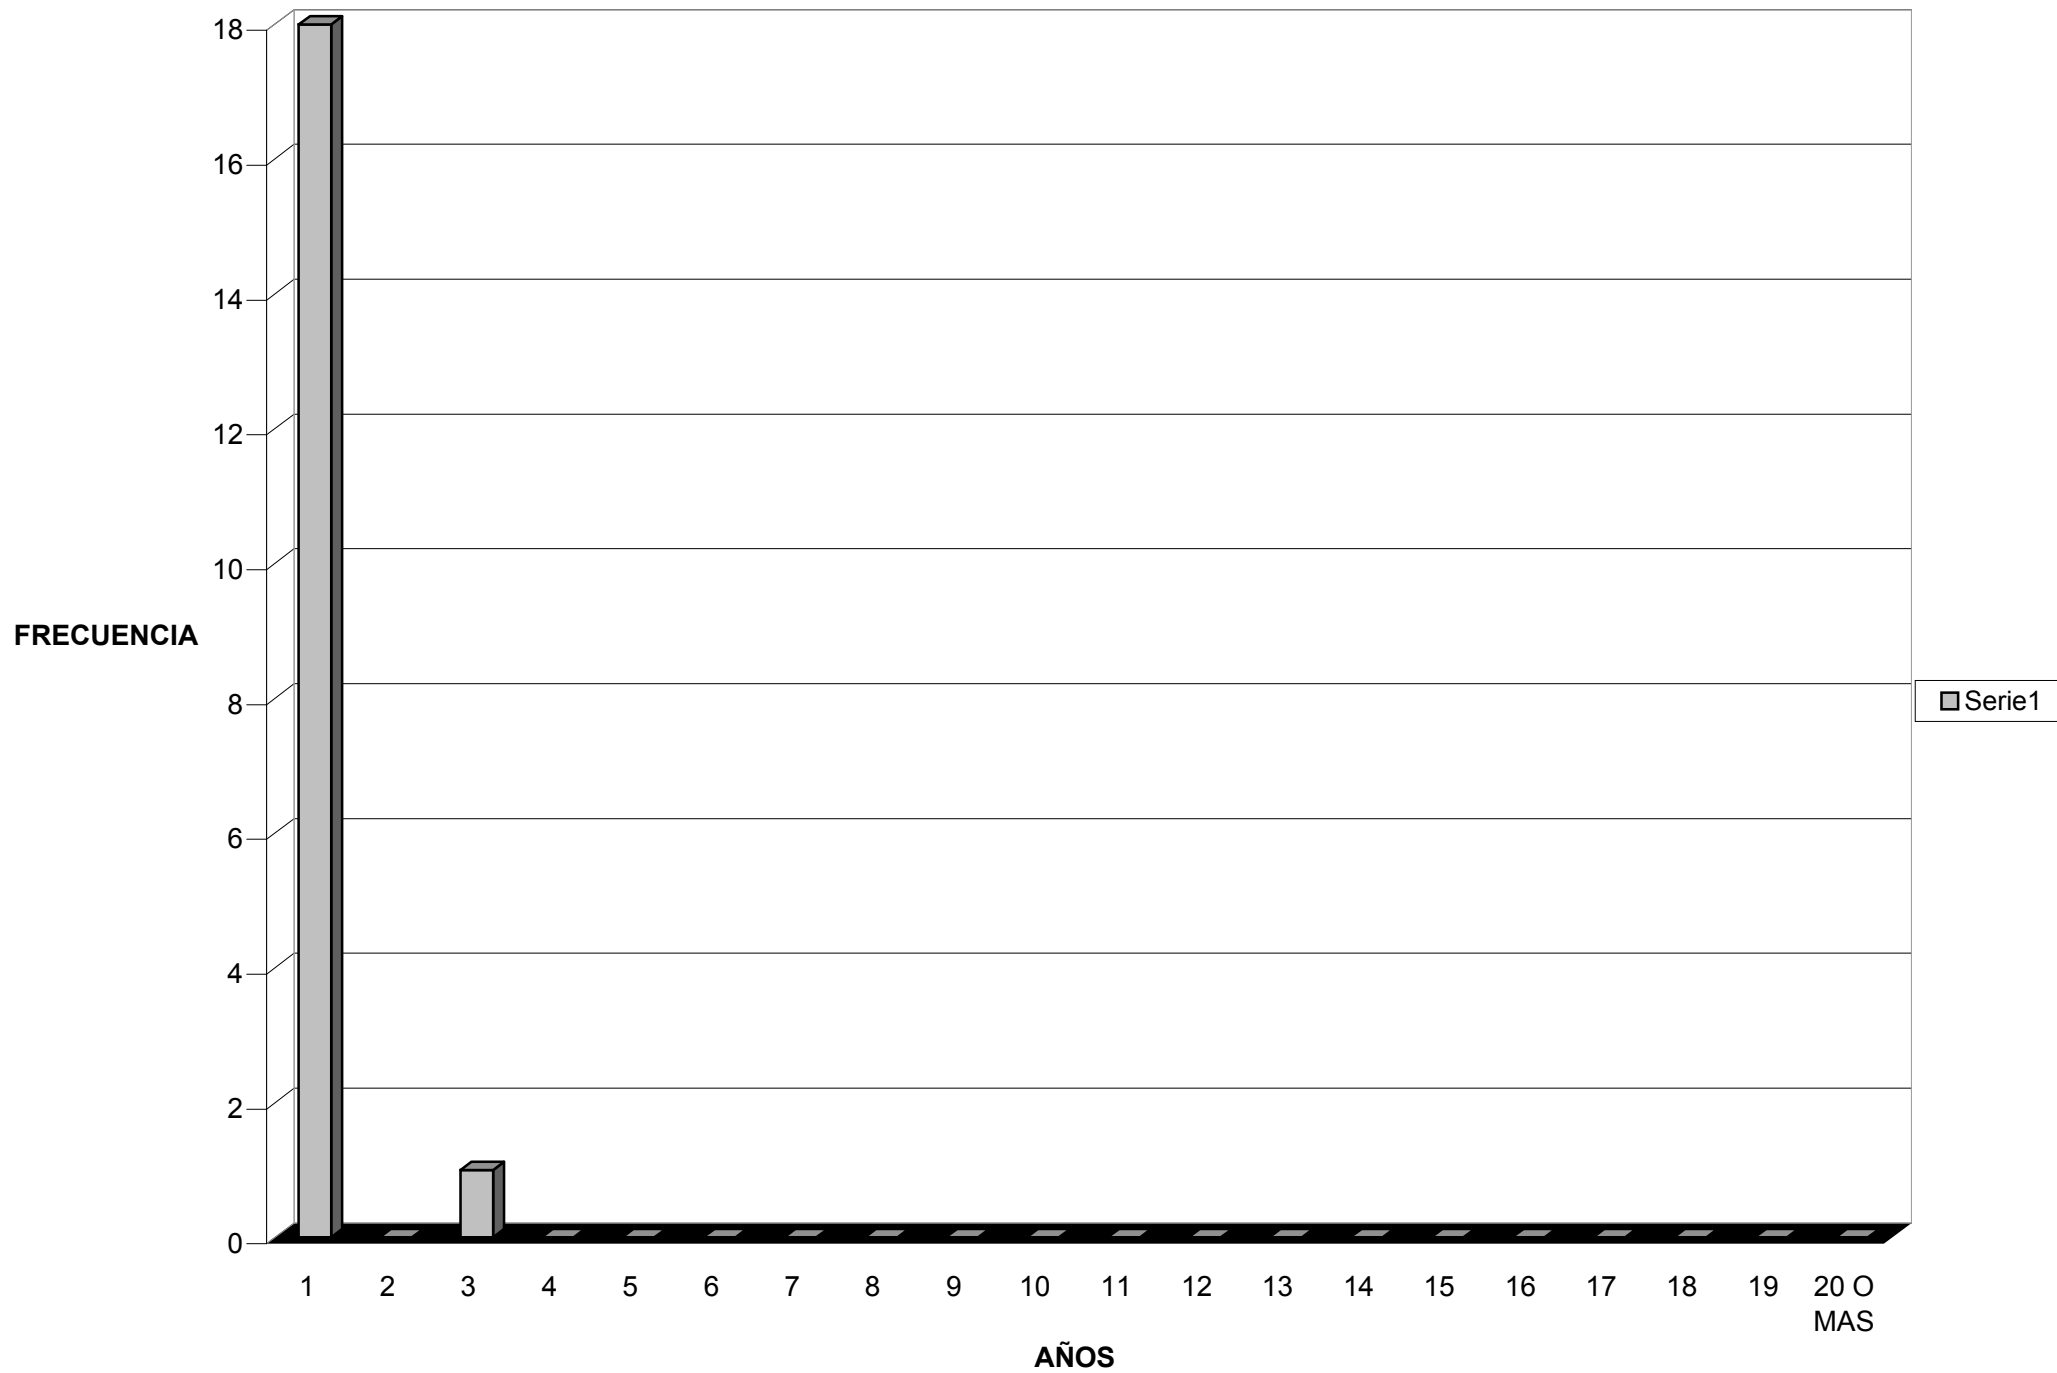


ASPIRADOR SIN MANTENIMIENTO RONDA-2

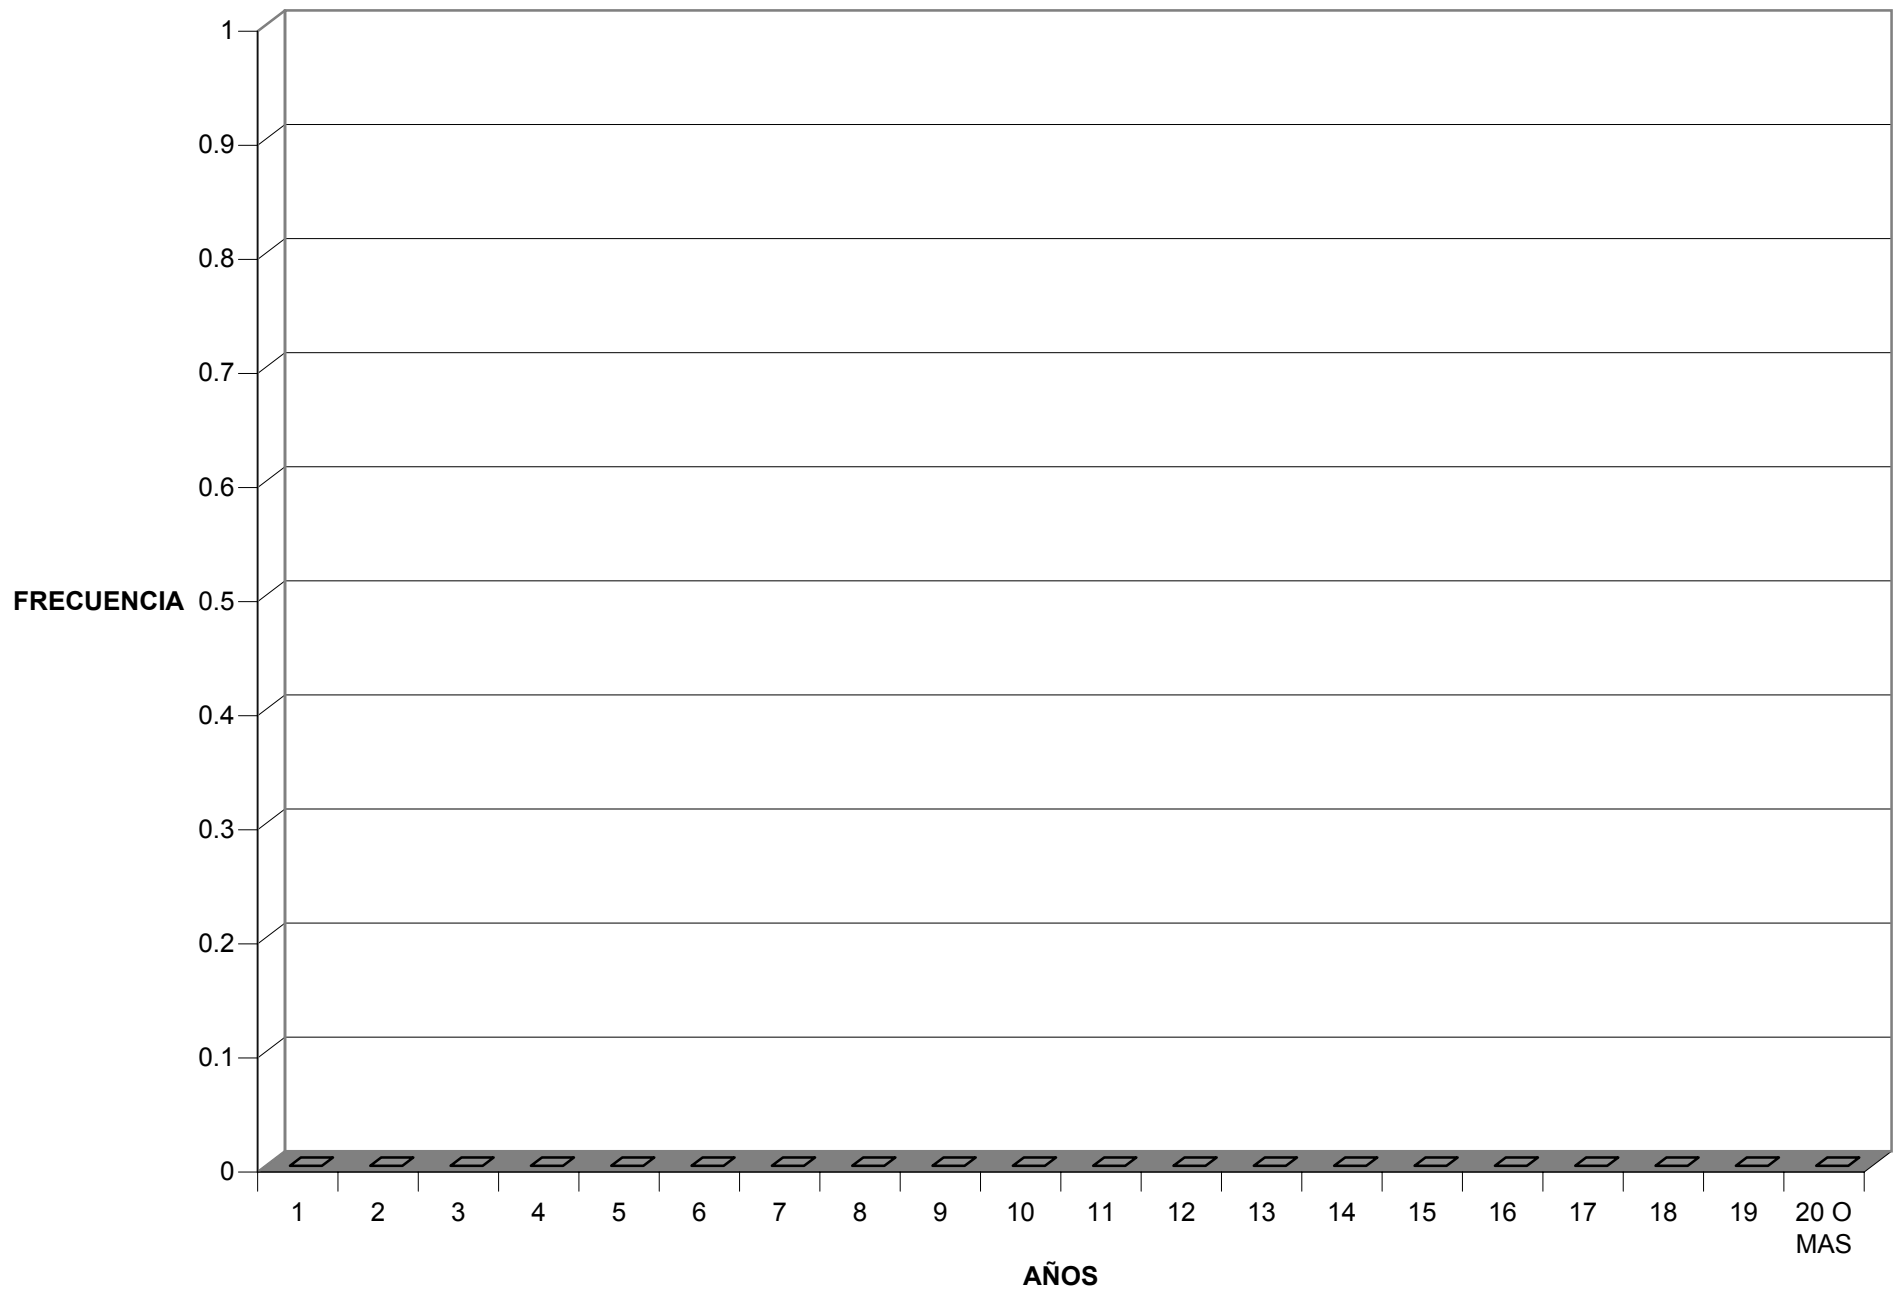


ASPIRADOR SIN MANTENIMIENTO RONDA-3

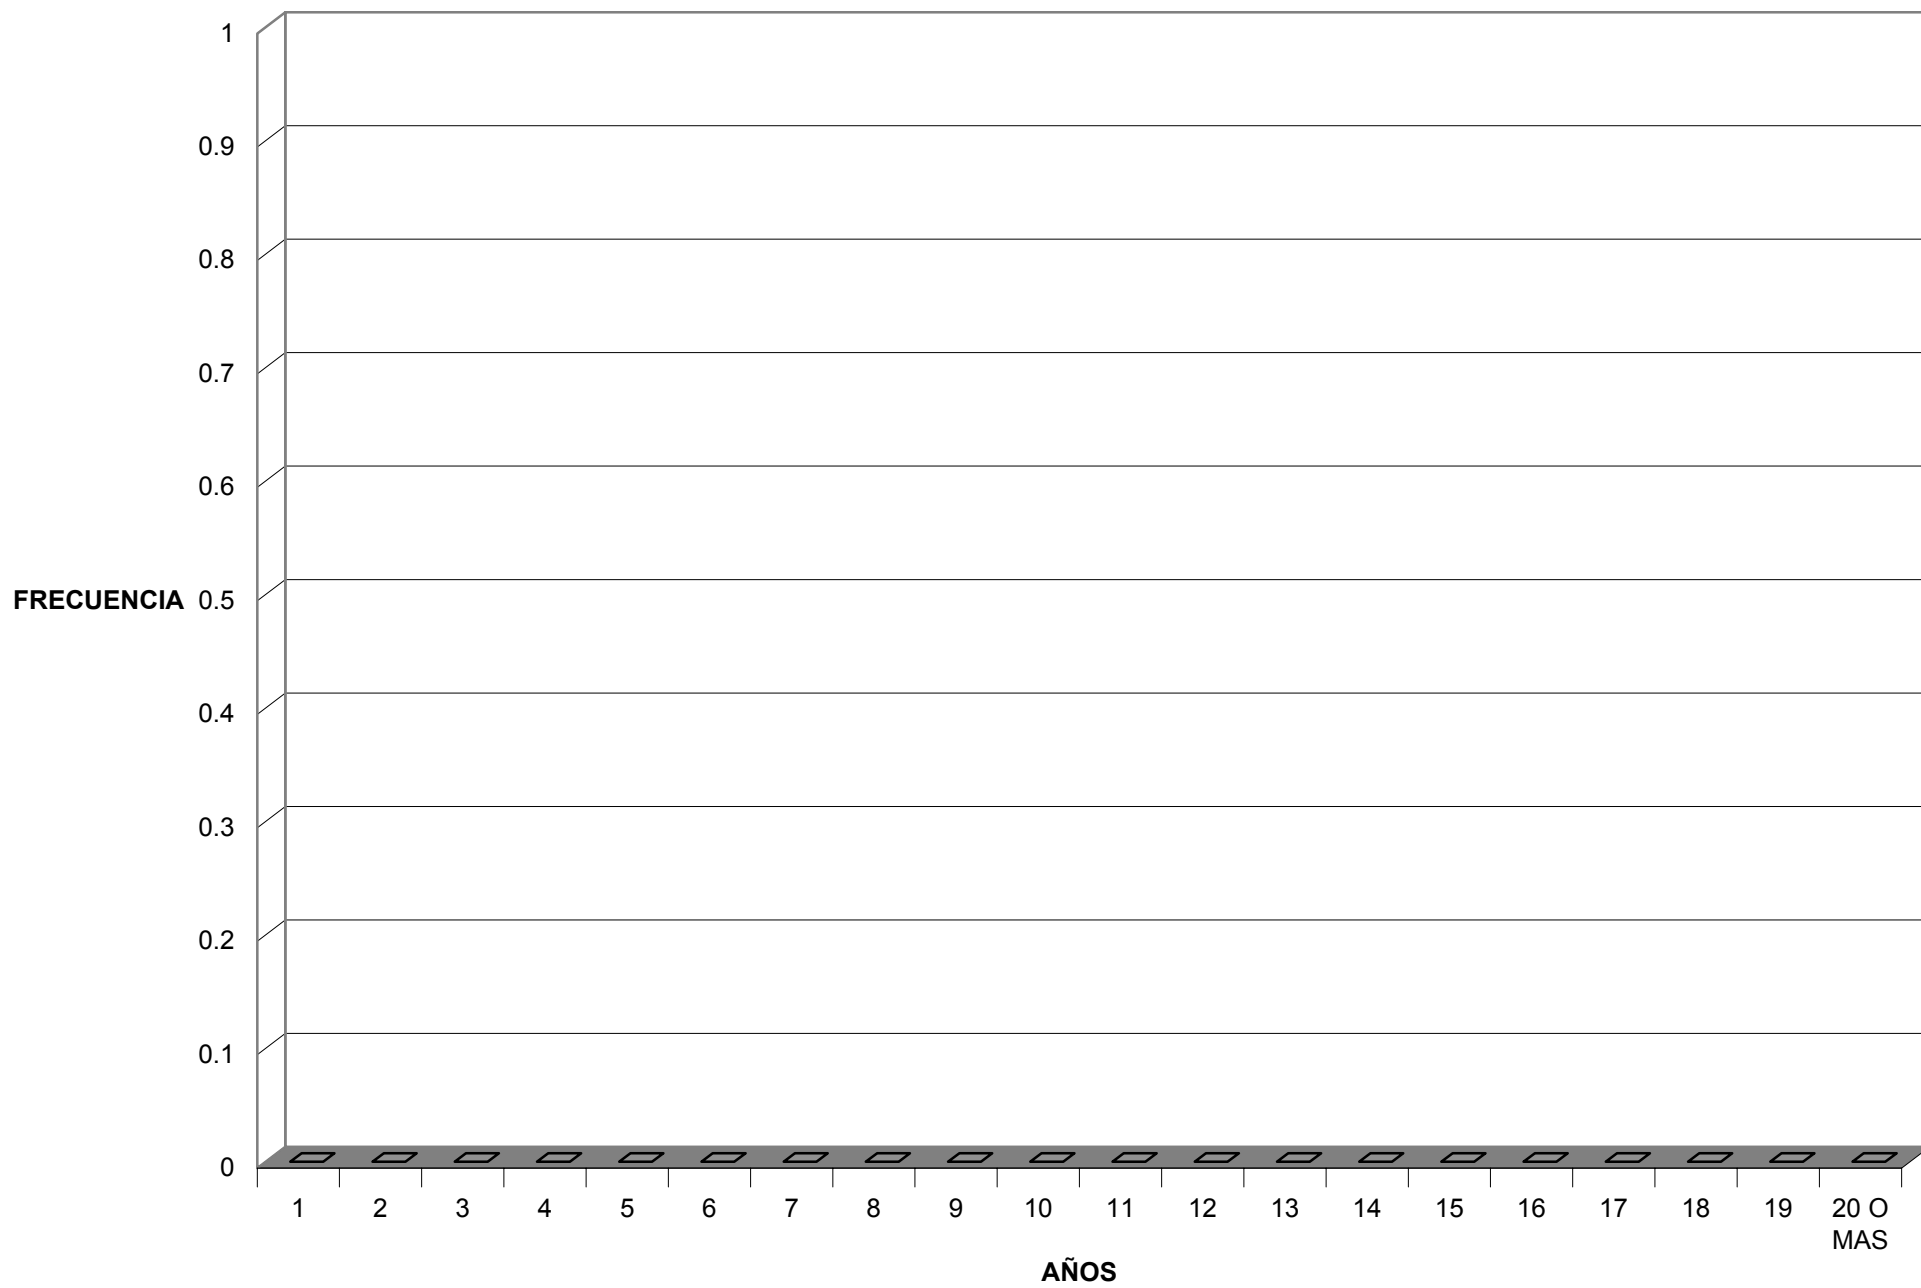

ASPIRADOR CON MANTENIMIENTO RONDA-1

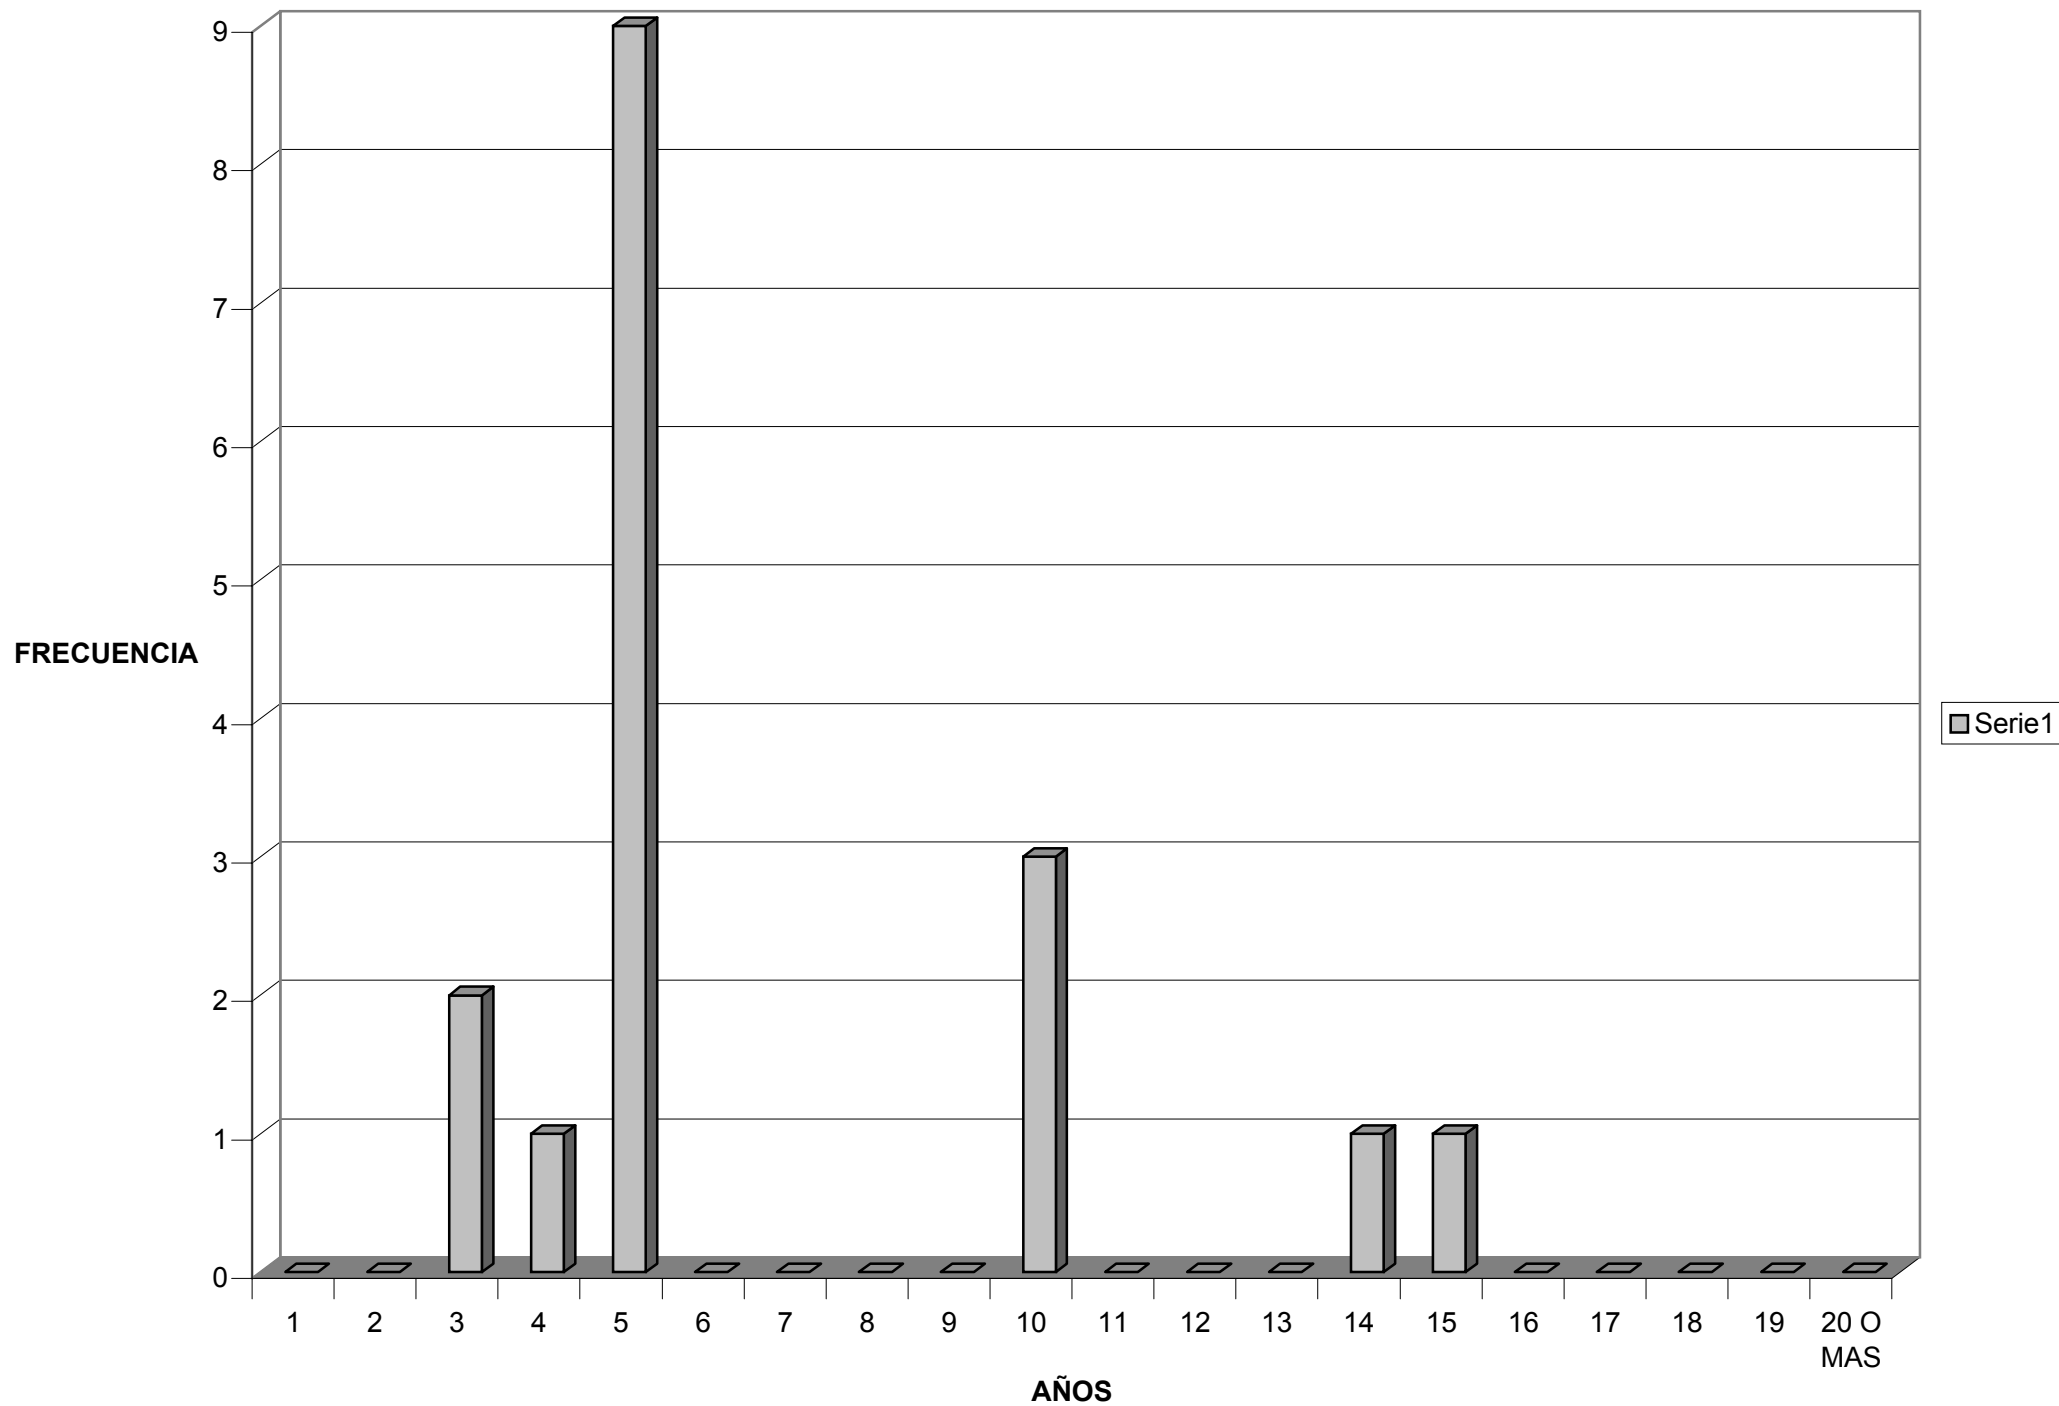

ASPIRADOR CON MANTENIMIENTO RONDA-2

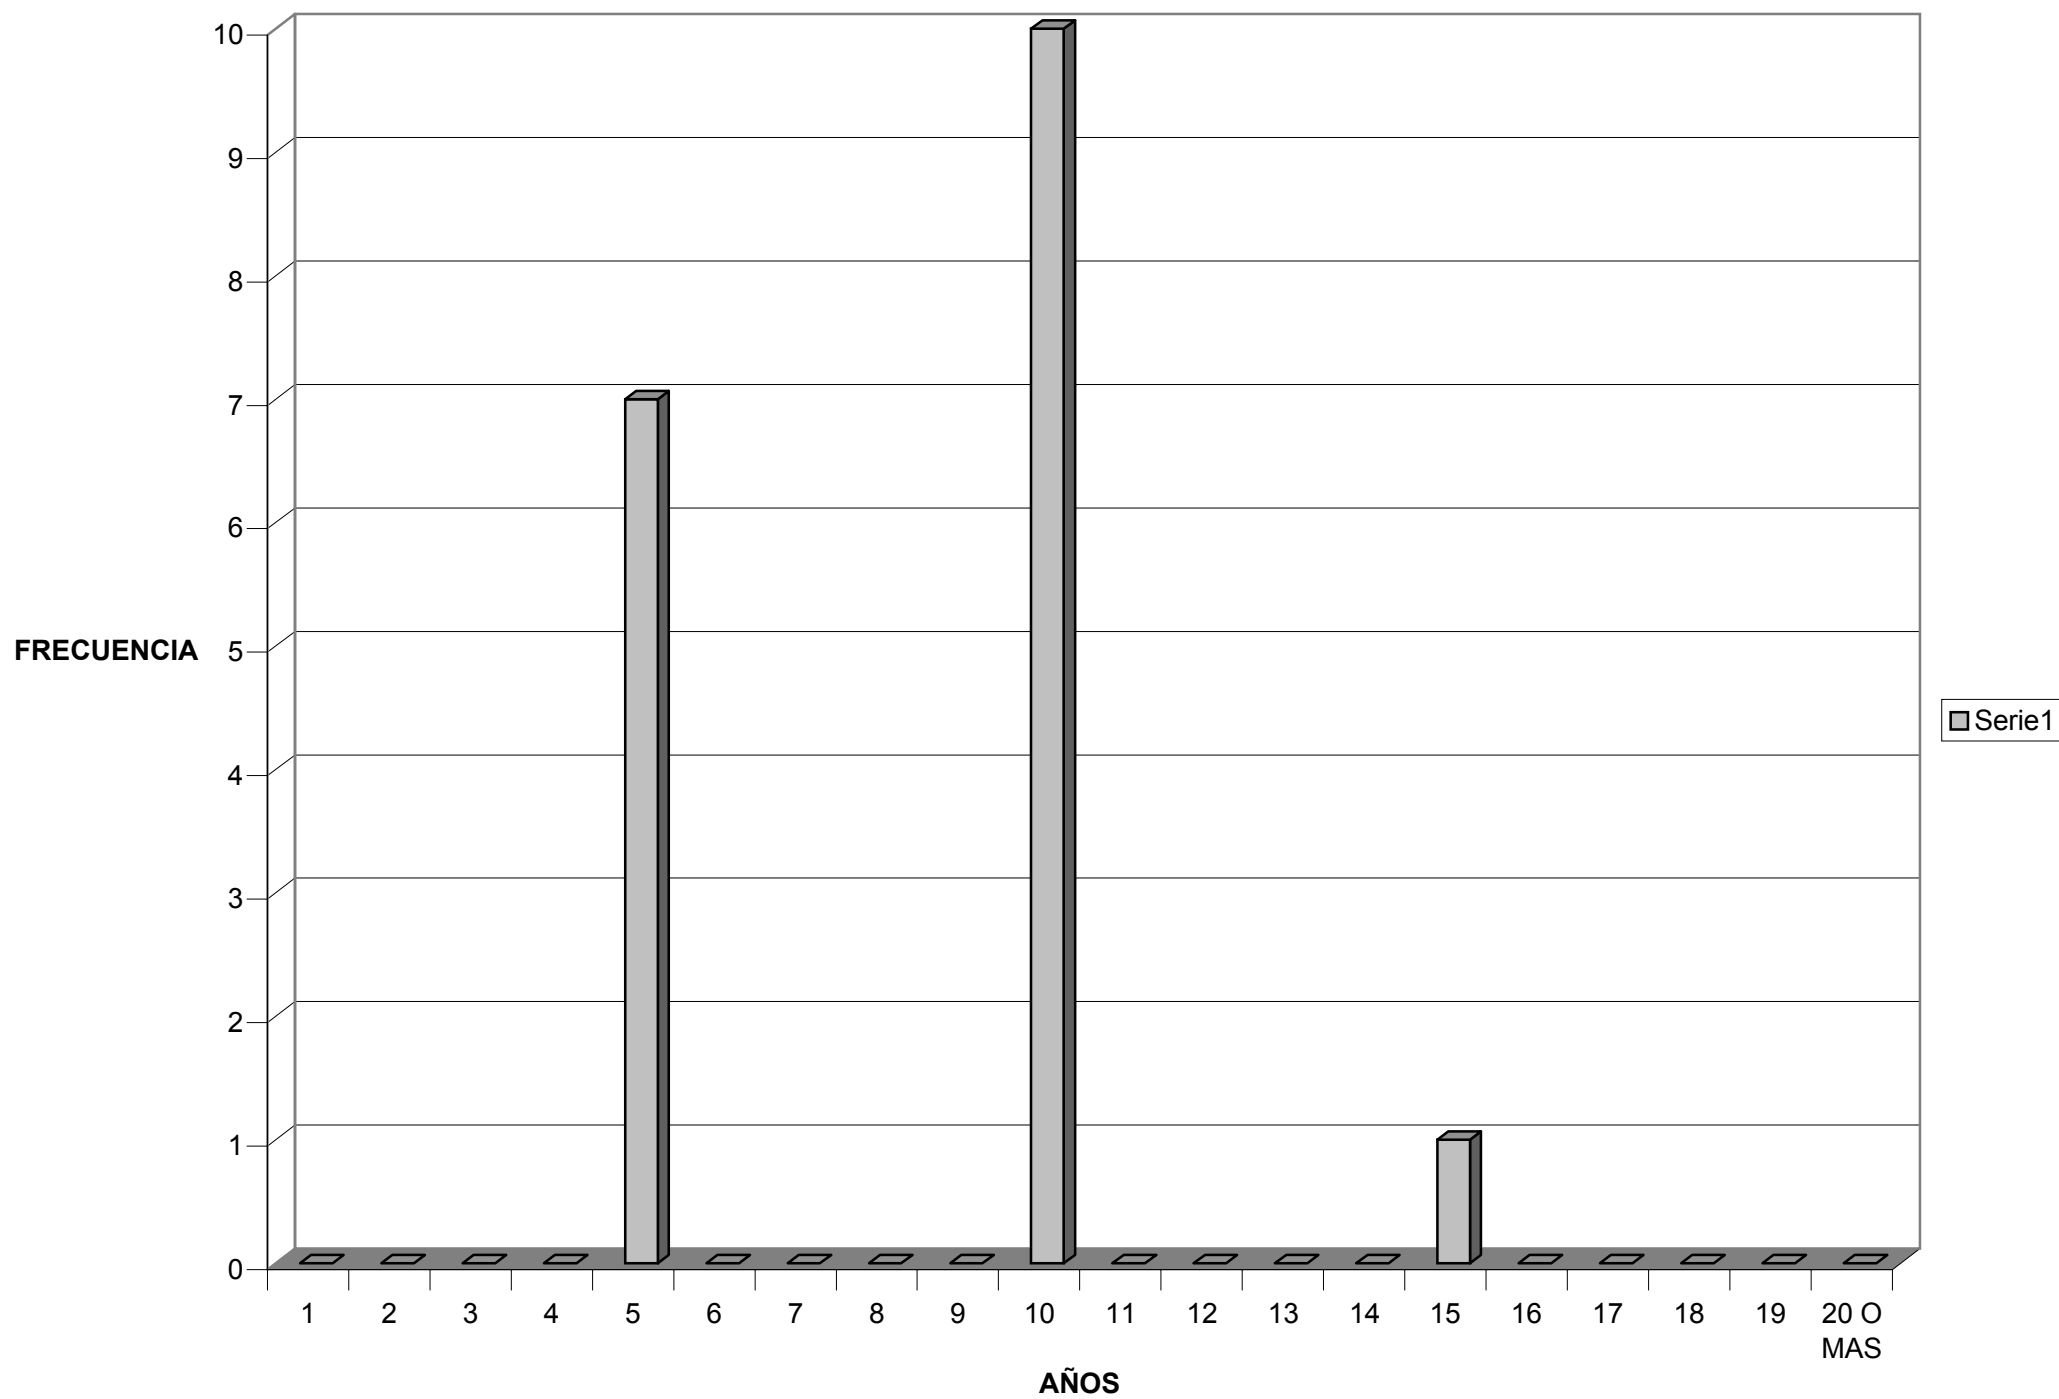

ASPIRADOR CON MANTENIMIENTO RONDA -3

